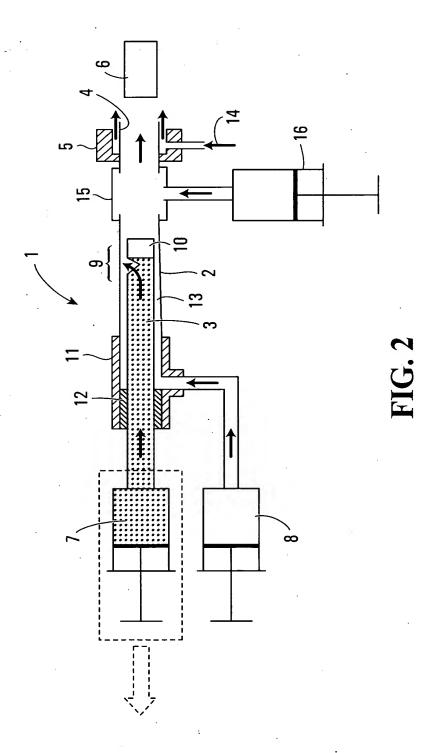


FIG. 1

Contact: Kevin R. Erdman Phone: 317.237.0300
CAPILLARY MIXER WITH ADJUSTABLE REACTION CHAMBER
VOLUME FOR MASS
APPLICATION NO. TO BE ASSIGNED

2/14



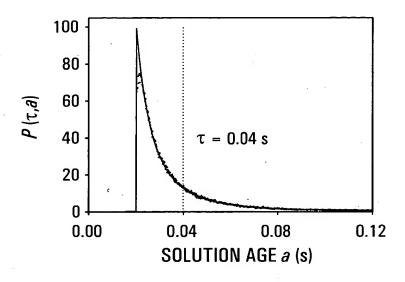


FIG. 3A

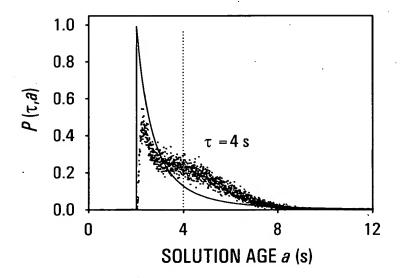


FIG. 3B

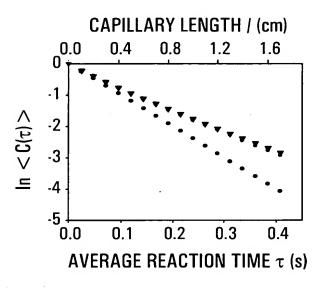


FIG. 4A

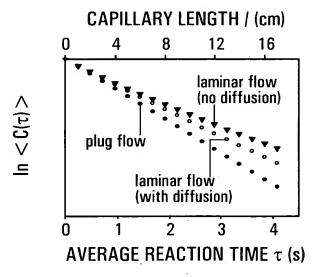


FIG. 4B

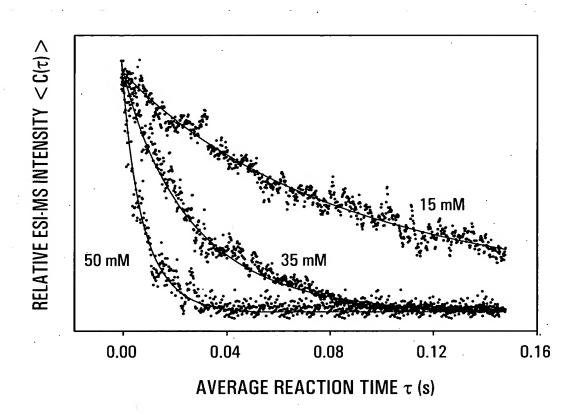


FIG. 5

APPLICATION NO. TO BE ASSIGNED


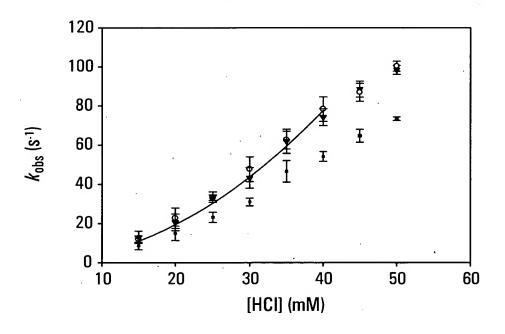


FIG. 6





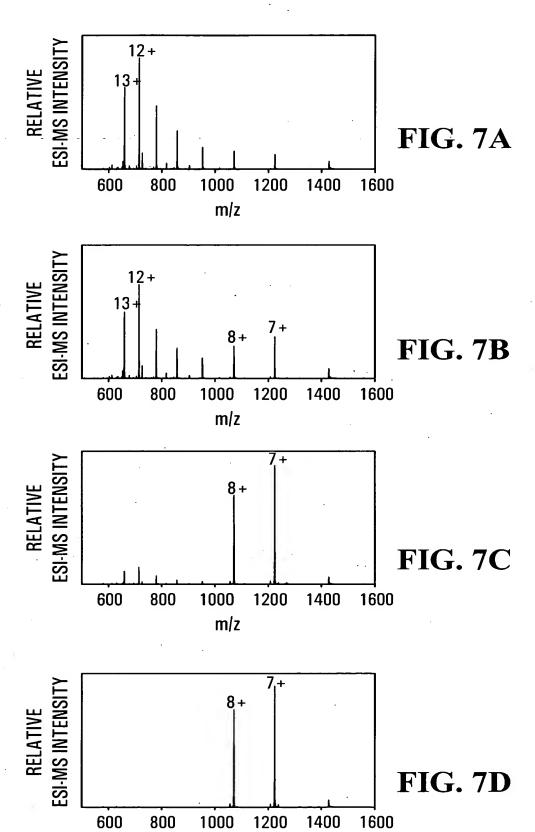

m/z

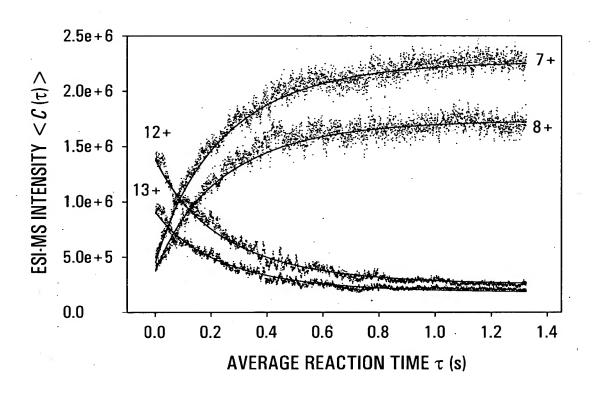


FIG. 8

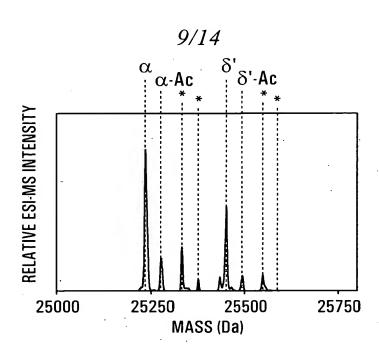


FIG. 9A

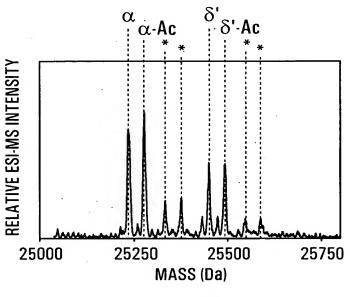


FIG. 9B

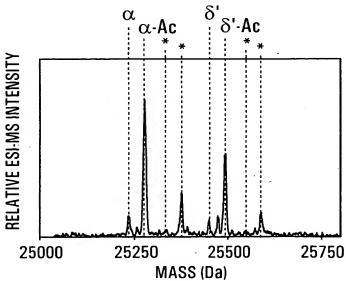


FIG. 9C

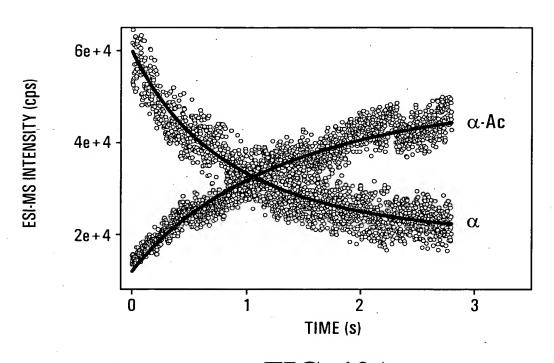


FIG. 10A

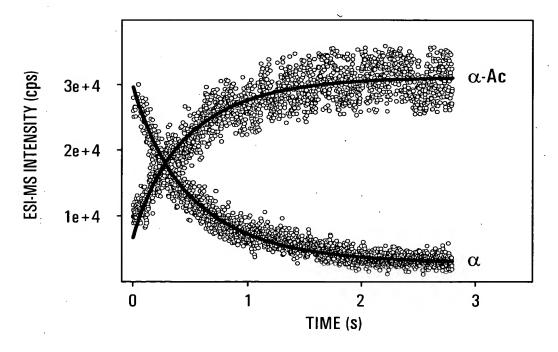


FIG. 10B

Contact: Kevin R. Erdman Phone: 317.237.0300
CAPILLARY MIXER WITH ADJUSTABLE REACTION CHAMBER
VOLUME FOR MASS
APPLICATION NO. TO BE ASSIGNED

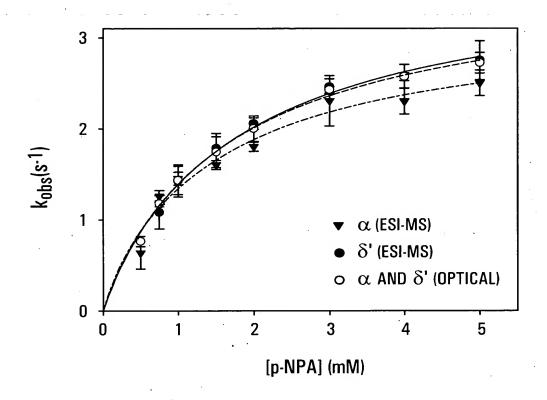


FIG. 11

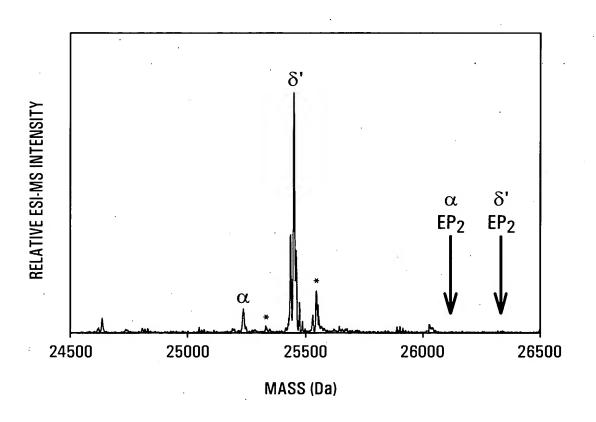


FIG. 12

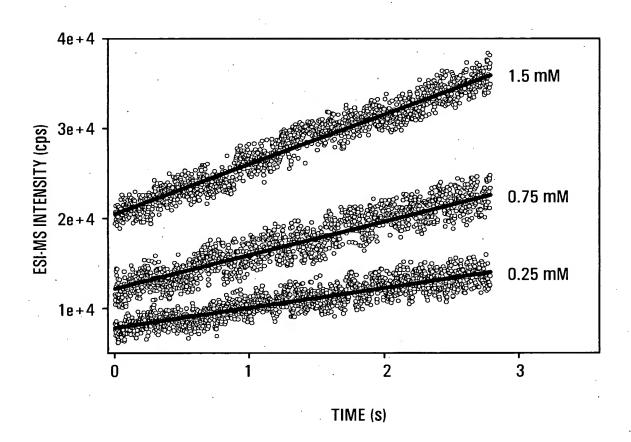


FIG. 13

Contact: Kevin R. Erdman Phone: 317.237.0300 CAPILLARY MIXER WITH ADJUSTABLE REACTION CHAMBER VOLUME FOR MASS APPLICATION NO. TO BE ASSIGNED

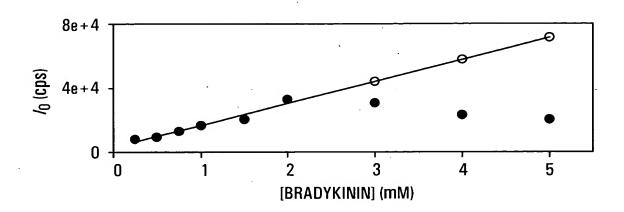


FIG. 14A

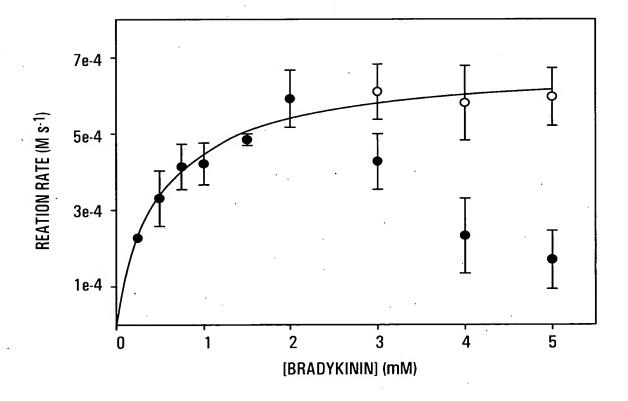


FIG. 14B